


**Supplementary Figure 1. Reproducibility of blood plasma clotting assay**

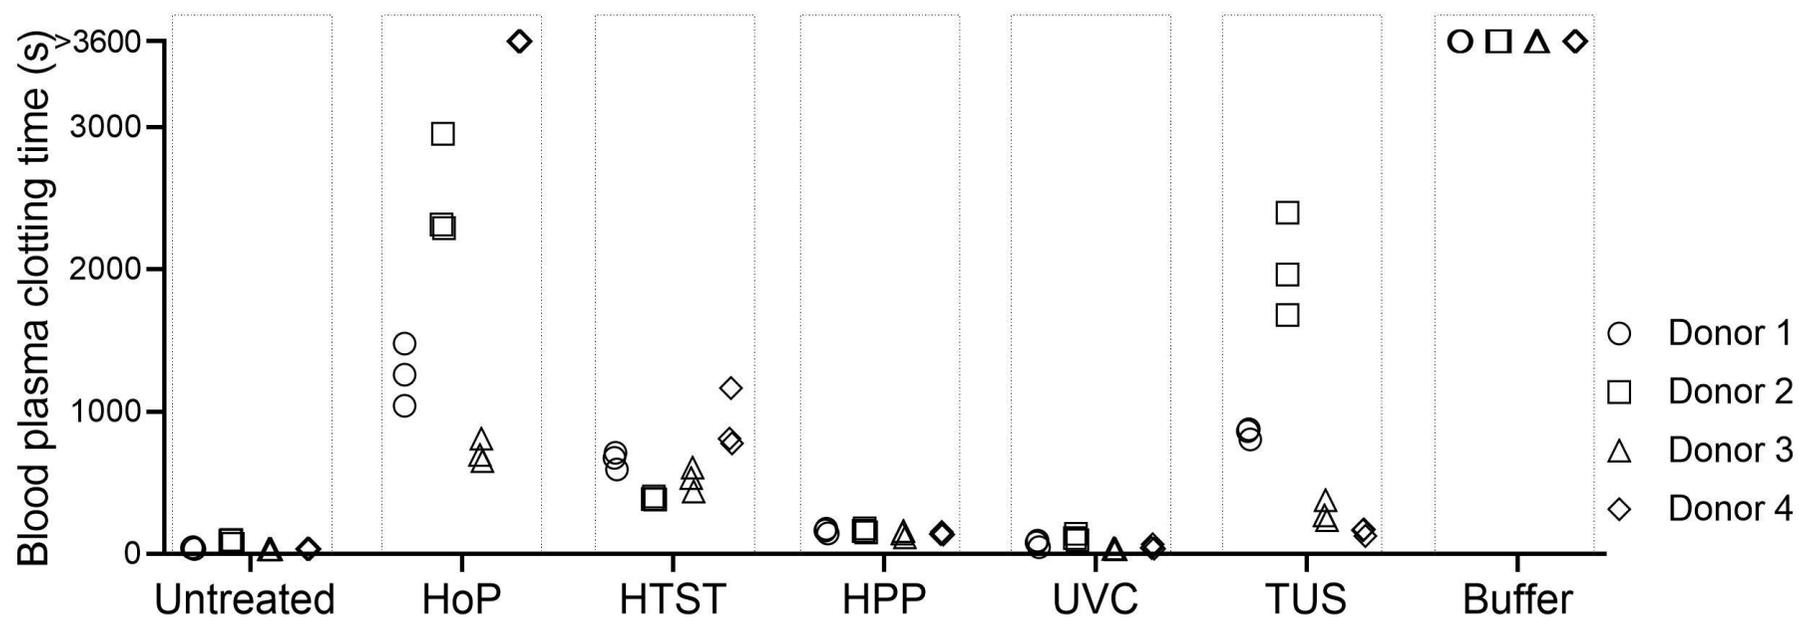

Human milk samples from randomly selected donors (n=4) were added to human blood plasma at the final concentration of 5 % (vol/vol) in triplicate. Saline was used as a negative control. HoP: holder pasteurization; HPP: high-pressure processing; HTST: high-temperature-short-time pasteurization; TUS: thermo-ultrasonication; UVC: ultraviolet-C irradiation. For each donor, a different symbol is used.